


LC-VS 60

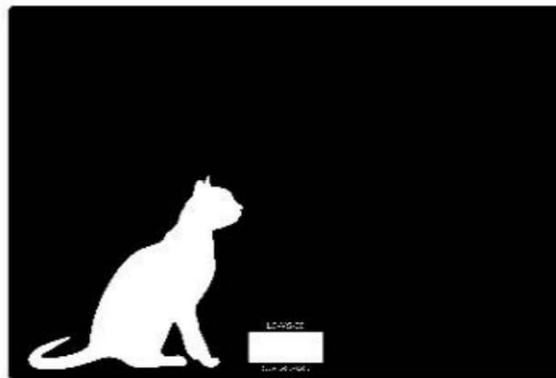

Operation Manual

Table of Contents

<u>Section</u>	<u>Page</u>
Declaration of Conformity	3
Customer Service	4
Introduction	4
Safety	5
Features	6
Application & Conformity	6
Getting Started	7
Delivery	7
Application Menu	8
Functions	9-11
Calibration	11
Maintenance & Service	12
Transportation & Storage	12
Warranty	13

Customer Service

USA

LW Measurements LLC,
620 Carlson Court
Rohnert Park, CA 94928
USA

Tel: (707) 542-2185
FAX: (707) 542-3285

<http://lwmeasurements.com>

EUROPE

LW Measurements Europe Ltd
Chalkwell Park House 700 London Road
Westcliff-on-Sea Essex SS0 9HQ
United Kingdom

Tel: 01702-476700
Fax: 01702-477380

<http://lwmeasurements.com>

Introduction

What you should know about these Operating Instructions:

Tree® Professional Weighing Equipment products are simple to operate.

Nevertheless, you should read through these operating instructions in their entirety, so that you can make optimum use of the full potential and the diverse possibilities of the weighing machine in your daily work.

These operating instructions contain guidance in the form of pictograms and keyboard diagrams, which should help you in finding the required information:

For the labelling of potential hazards and advice, please see Safety below.

Features

Model number	Capacity	Division
LC-VC-60	60lb	0.02lb
Platter / Tray	25 x 16inch/63×40mm	
Net/gross weight	12.3 lb/15.4 lb. / 5.6kg/7 kg	
Package	Standard carton:720x490x115 (mm ³)	
Operating Temperature	Optimum: 15-30C (62-90F)	
Indicator	4×AA Batteries or AC/DC	
Power source	Adapter 6-9V /300mA	

- Auto shut off (optional)
- Auto zero tracking
- Large LCD
- Large square weighing tray.
- Auto calibration
- AC Power
- Hold function
- Auto backlight (optional)

Application & Conformity

The weighing scale may only be used for the weighing of solid-materials and of liquids filled into secure containers.

The maximum capacity load of the weighing scale must never be exceeded, otherwise the weighing scale may be damaged.

In using the weighing scale in combination with other devices as well as with devices produced by other manufacturers, the appropriate regulations for the safe use of the relevant attachments and their application in accordance with instructions must be observed.

The weighing scale has been manufactured and tested in accordance with the standards and recommendations set out in the declaration of conformity.

The power adapter supplied for the weighing scale complies with the appropriate electrical protection class.

Getting Started

The scale is packaged in an environmentally-friendly carton, which provides optimum protection for the balance during transportation.

We suggest that you keep the original packaging in order to avoid damage if you are shipping or transporting the scale to a different location. It is also the best way to keep it in the best conditions if it will not be used for an extended period of time.

In order to avoid damage, please follow the instructions provided below, when unpacking the scale:

- Unpack the scale carefully.
- When outside temperatures are very low, the scale should be stored for a couple hours and kept in its box in a dry room at normal temperature, so that no condensation settles on the unit when opening the box.
- Check the scale immediately after unpacking for any external visual damage. If there is any damage on scale, contact customer service immediately.
- If the scale is not to be used immediately after purchase, it should be stored in a dry place where fluctuations in temperature are low. (Reference pg.).
- Read through these operating instruction, before you work with the unit and pay attention to the Safety recommendations (reference Safety pg. 6).


Delivery

Inspect delivery for completeness immediately on unpacking all components.

Checklist for complete delivery

	Component delivered present yes / no
Weighing unit body	
Rubber mat	
Remote display (optional)	
Power adapter	
Operating manual	


Application Menu

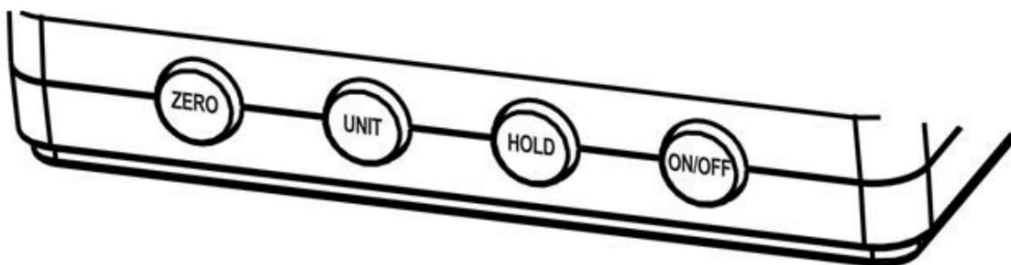


Key Descriptions

- ON/OFF : Press the key to turn the scale on or off
- HOLD: Press this key to store weight value
- UNIT: Select weighing unit: kg and lb.
- ZERO/TARE: To deduct the weight of the container such as pan on the scale and the tared range is up to 100% of full capacity.

Display

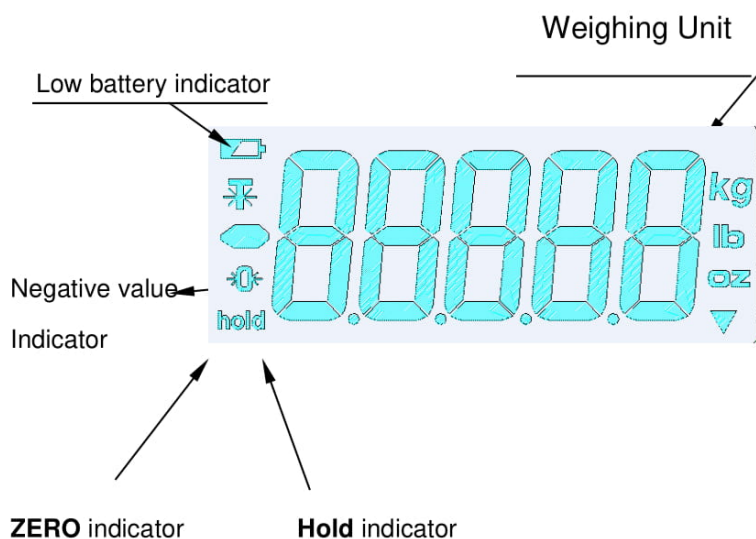

Indicates when the reading is 0

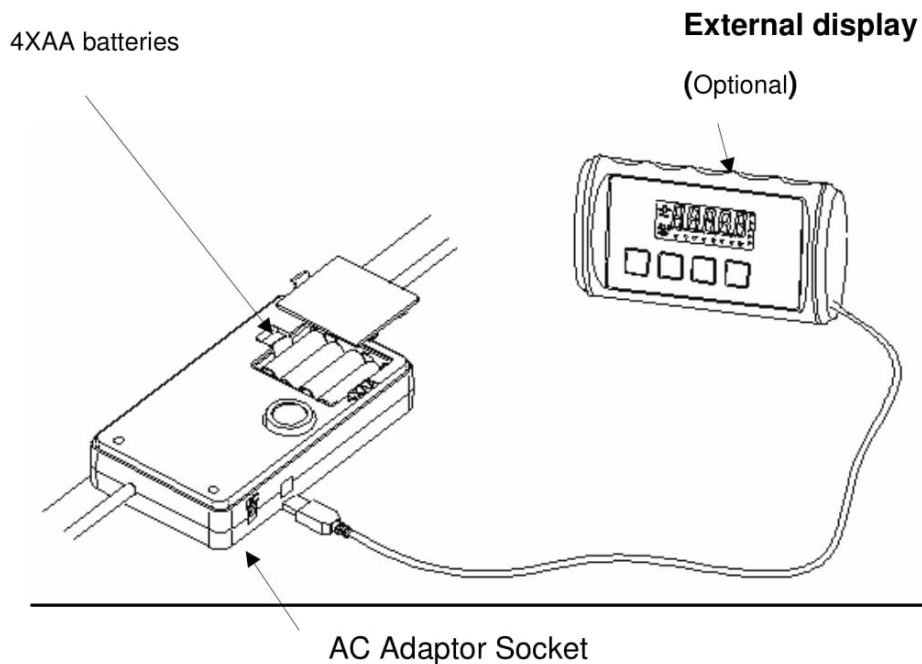

Functions

HOLD FUNCTION


- Place the item on the scale platform.
- Wait for the weights to be displayed.
- Press the [HOLD] key. The “hold” hold indicator will turn-on.
- Remove the item from the scale platform. The item’s weight reading will remain on the display. You can now also convert this to other measures (i.e. to pounds, pounds & ounces or kilograms) by pressing the [UNIT] key.
- Quit hold function: Once an item is weighed and the hold function is enabled; you want to quit to hold function, Press the [HOLD] key again to cancel the “hold” hold indicator and return the scale to weight mode.

WEIGHING

Before weighing

Whenever possible, please allow the scale to warm up for one minute after first turning the power on so that the scale will function properly and accurately.

Error messages

 : Low battery

Err-0: Overload

Err-Z : Exceed zero track range when turn on the power

Err- S: The scale is unstable when turn on the power

Err- C: Forget to input calibration weight when calibrating or the AD value is too low.

Weighing procedures

Press [ON/OFF] to turn on the scale.

When the power is turned on, all display segments appear for a few seconds and "0" will appear on the display.

Select the weighing unit with [UNIT].

Press [UNIT] to select a weighing unit "kg", "lb".

Once the unit has been selected, the selected unit will be displayed next to the weight value.

Start weighing

If you do not use a container for weighing,

Verify the reading is "0". If not, press [ZERO] to display "0".

Place the items to be weighed on the platform.

If you use a container for weighing

Place an empty container on the platform.

Wait for the stability weighing to be displayed and press [ZERO].

Place the objects to be weighed in the container.

FUNCTION SETTINGS

- Enter function setting mode. Press [ON/OFF] to turn the power off, Press [ZERO] first, then press [ON/OFF], while keeping [ZERO] pressed, the display will show **A_OFF**.
- Selection of auto shut off mode. When the scale enters function setting menu, the display will show **A_OFF**. Press [ZERO] to choose ON or OFF: selection display **ON**, this means auto shut off function active. Press [ZERO] again, the display will show **OFF**, this means auto shut off function inactive.
- Selection of auto backlight mode. When the scale enters function setting menu, press [UNIT] key, the display will show **L-ON (or OFF)**. Press [ZERO] to choose

ON or OFF: selection display **ON**, this means auto backlight function active, press **[ZERO]** again, the display will show **OFF**, this means auto backlight function inactive, i.e. shut off backlight function.

- Selection of auto HOLD mode. Press **[UNIT]** key, the display will show **H_ON** or **H_OFF**, press **[ZERO]**, selection display **H_ON**, this means **AUTO-HOLD** function active, press **[ZERO]** again, the display will show **H_OFF**, this means **AUTO-HOLD** function inactive.
- Return to weighing mode. Press **[ON/OFF]** to turn the power off, press **[ON/OFF]** again to turn on the power and the scale return to the weighing mode.

Calibration

When to calibrate

If the scale is inaccurate, calibration may be desired when the scale is first set up for use, or if the scale is moved to a different altitude or gravitation. This is necessary because the weight of a mass in one location is not necessarily the same in another location. Also, with time and use, mechanical deviations can occur.

How to calibrate

Note: calibration value must be at least half the weight (30 lb.) that you have set.

1. Press and keep **[UNIT]** key then press **ON/OFF** key to turn on the scale, the display will show **CAL** then **AD** value.
2. Press **[UNIT]** key, the display will show flashed calibration weight. Place the shown weight then press **[UNIT]** key, the display will show ----- then **AD** value.
3. Take off calibration weight then turn off the scale. Calibration is finished.

If calibration is repeatedly incorrect then: 1) Replace the batteries, 2) Try a more stable surface or vibration and interference free location.

Maintenance and service

The weighing machine must be treated carefully and cleaned regularly. It is a precision instrument.



DANGER

For maintenance-work, the balance must be disconnected from the power supply (remove power adapter plug from socket). Also ensure that the balance cannot be connected to the power supply during the work by a third party.

Make sure that no liquid spills into the scale while performing maintenance work. If liquid is spilled on the scale, it must be inspected by a service technician.

Regularly perform maintenance to the weighing pan and the weighing pan holder by removing any dirt or dust from under the weighing pan and on the weighing scale housing. Use a soft brush or a soft, lint-free cloth, moistened with a mild soap solution.

Never use solvents, acids, alkalis, paint thinners, scouring powders or other aggressive or corrosive chemicals for cleaning; these substances can cause damage to the



CAUTION

Transport & Storage

Your weighing machine is a precision instrument, treat it carefully. Avoid shaking, severe impacts and vibration during the transportation. Make sure that there are no marked temperature fluctuations during the transportation and that the weighing machine does not become damp (condensation).

If you would like to take the weighing machine out of service for an extended period, disconnect it from the electricity supply, clean it thoroughly (refer to Maintenance & Service) and store it in a place which meets the following conditions:

- No violent shaking, no vibrations
- Minimum temperature fluctuations
- No direct solar radiation
- Minimum moisture

Warranty

The products are under warranty against factory defects for a period of two (2) years from the date of shipment.

For Customers within the lower 48 states of the continental United States. LW Measurements will pay for freight both ways for the first 30 days after purchase. After 30 days expire the customer is responsible for shipping the product back to us. After the product is received we will inspect it and as necessary we will repair or replace and will ship the product back to the customer at our expense.

Any new scales returned for warranty must be properly packaged in the original box. If they are not properly packed an in the original box, the customer pays for shipping cost. If we determine there is a factory defect, we will pay for the shipping back. If we determine that it is not a factory defect, the customer will pay shipping.

For Customers outside the lower 48 States, including Mexico, Canada, Puerto Rico, Hawaii, Alaska and all other countries, customers must pay for shipping.

Our warranty does not cover misuse or neglect including but not limited to battery or water damage, overloading, and chewed or cut wires. If the product is found to have been misused or damaged by the customer, LW measurements is not responsible for the cost of return.

For warranty claims please go online to lwmeasurements.com and fill out the warranty submission form or call your customer service representative.