


FBx Series Bench Scale Instruction Manual

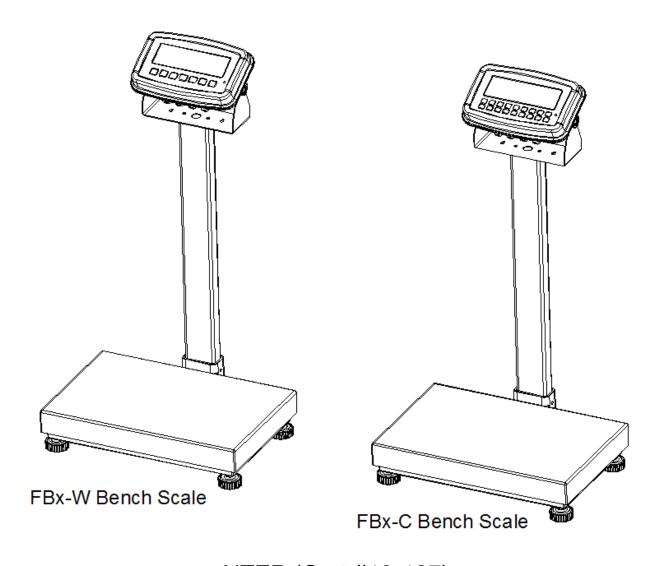

NTEP (Cert.#19-137)

Fuzhou Furi Electronics Co.Ltd

1. Description

This manual contains installation, operation and maintenance instructions for the FBx Series Bench Scales. Please read this manual completely before installation and operation.

The indicator instructions please refer to "FBx Indicator Manual".

The FBx Series is a dedicated static checkweighing product line with enhanced software and simplified user functionality. FBS is stainless steel construction. Its easy-to-clean, hygienic design makes it specifically ideal for food processing and other wet-environment applications.

Behind this instrument stands Furi, An Aftermarket Department with trained instrument technicians is dedicated to providing the fastest service possible in the event this instrument requires servicing. Furi also has a Customer Service Department to answer any inquiries regarding applications and accessories.

1.1 Precautions




For safe and dependable operation of this equipment, please comply with the following precautions:

- Verify that the input voltage range printed on the data label matches the local AC power to be used.
- Make sure that the power cord does not pose a potential obstacle or tripping hazard.
- Use only approved accessories and peripherals.
- Operate the equipment only under ambient conditions specified in these instructions.
- Disconnect the equipment from the power supply when cleaning equipment.
- Do not operate the equipment in hazardous or unstable environments.
- Do not immerse the equipment in water or other liquids.
- Service should only be performed by authorized personnel.

1.1.1 Power Adapter Option Safety Precautions

Please use only approved Power Adapter.

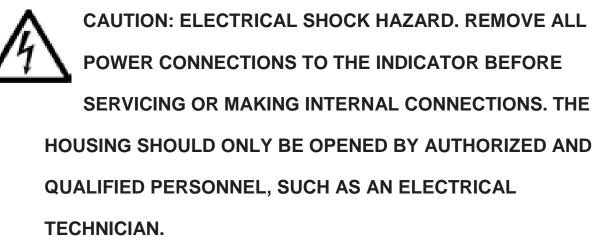

Before making connections to the Power Adapter, remove power from the system. If the system contains an optional rechargeable battery, be sure that the button is used to fully turn off the system after removing the AC power plug.

More detailed installation instructions are included with the Power Adapter when purchased.

2. INSTALLATION

2.1 Unpacking and Checking

Unpack and verify that the following components have been included:

FBx bench scale

Instruction Manual

Certification/Packing list

Stainless Steel platform

Accessory pouch

Warranty Card

Retain all of the original packaging materials in the event the unit has to be transported or stored.

2.2 Precautions

- •This equipment should be used in an environment free from vibration, temperature extremes or highly corrosive conditions.
- •These factors may affect normal operation of the unit.
- •Scale bases used with the FBx Indicator must be located on a stable level surface and kept away from vibrating sources such as large machinery or appliances.
- •Adjust the leveling feet so that the bubble is centered in the circle of the level indicator located in the rear of the scale.

Note: Ensure that the scale is level each time its location is changed.

2.3 Power Connection

2.3.1 Power Adapter

Plug the AC power cord into a properly grounded power outlet. The FBx Indicator utilizes a universal switching power supply, AC 100-240V 50/60Hz Input, DC 12V 1000mA Output.

2.3.2 Battery Power

The scale can be operated on the internal rechargeable battery when AC power is not available. The scale will automatically switch to battery operation if there is a power failure or the power cord is removed. A fully charged battery can operate the scale for over 16 hours independent of the AC power line.

When the battery requires charging, Low Battery Indicator is displayed during operation. When the battery is fully discharged LCD will display turn off. At this time, please recharge in time, otherwise the scale will not be able to continue to use.

With AC power applied to the scale, a Yellow led may light up, which

means charging is in progress. Turning to a green led indicates that the battery is fully charged.

It's not necessary to turn on the power when the scale is during charging process. It takes 3 hours at least to charge the battery fully.



Before using the scale on battery power for the first time, the internal rechargeable battery requires charging for up to 10 hours. The scale can be operated on AC power

adapter during the charging process. The battery is protected against over charging and the scale can remain connected to the AC power line.

Λ

CAUTION


BATTERY IS TO BE REPLACED ONLY BY AUTHORIZED SERVICE PERSONNEL.

RISK OF EXPLOSION CAN OCCUR IF REPLACED WITH THE WRONG TYPE OR CONNECTED IMPROPERLY.

2.4 Before Weighing

Whenever possible, allow the scale to warm up more than thirty (30) minutes. This gives the scale a chance to adjust to its new environment.

3.1 Drawings and Dimensions

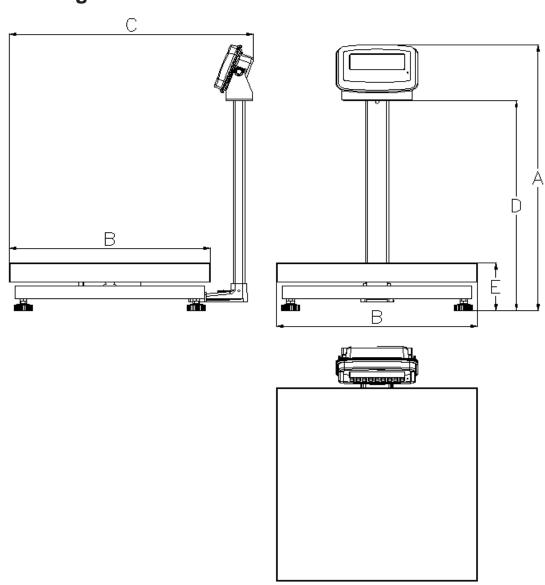

	Α	В	С	D	E
Base	Total Height	Total Wdth	Total Length	Dimension from Indicator bottom to the ground	Dimension from Platform surface to the ground
FBx-m1824	33inch	18inch	29inch	26inch	6inch
FBx-m2424	33inch	24inch	29inch	26inch	6inch

Figure 3-1. FBx Series Bench Scale.

3.2 Technical Data

Materials

• Indicator Housing: Stainless steel

• FBS scale structure: stainless steel; FB scale structure: cast steel

Keypad/display overlay: Polyester

• Feet: Rubber

Ambient conditions

The technical data is valid under the following ambient conditions:

Ambient temperature: -10°C to 40°C / 14°F to 104°F

Relative humidity: Maximum relative humidity 80% for temperatures up to 31°C decreasing linearly to 50% relative humidity at 40°C.

Height above sea level: up to 4000m

TABLE 3-1. TYPICAL CAPACITY AND GRADUATION VALUES

Model	Capacity	e min	Platter size
FBx-m1824	500lb 8000oz 226.80kg 226800g	0.1lb 2oz 0.05kg 50g	18inch x 24inch
FBx-m2424			24inch x 24inch
FBs-m1824			18inch x 24inch
FBs-m2424			24inch x 24inch

Explanation of model designations: FBx-myyyy;

x: denotes the material

S indicates Stainless Steel and blank indicates Cast Steel;

m: denotes the indicator model, where

- C denotes the indicator with number keys and
- W indicates the indicator without number keys;

where blank indicates scale structure model;

yyyy: denotes the platter size in inch (ex-1218 indicates 12inch x 18inch);

3.3 Calibration

The FBx scale is shipped pre-calibrated from the factory. However, many

conditions may require that the scale be recalibrated. Temperature changes, geographic gravity variations and rough handling are few reasons why a scale may need recalibration.

Notes: 1. Make sure that appropriate calibration masses are available before beginning calibration.

- 2. Make sure that the scale is level and stable during the entire calibration process.
- 3. Calibration is unavailable with J13 interface is not shorted CAL

- 4. Allow the scale to warm up for more than thirty (30) minutes after stabilizing to room temperature.
- 5. To abort calibration, press key anytime during the process.

3.3.1 Any Value Calibration (AnyCal)

AnyCal Calibration uses two points to adjust the scale. One point is called the zero value where there is no weight on the scale. The other point is any value that can be set, but it is recommended that the value is not less than half of the full capacity. The value closest to the full capacity is recommended to give the best performance over the entire weighing range.

Follow the steps below to calibrate the FBx scale:

Step 1: To enter the parameter menu mode:

• Open the indicator housing. Shorting the CAL jumper of J13 on the main

PC board. See GAL

1 2 3 J13

Move to position 2-3

• Press key to turn on the indicator, the system will enter the self checking mode.

• Press key during appears on the display, the display will show. The CAL arrow is lighted until the CAL jumper of J13 is removed and moved over to the left.

Press key to select the setting menu in menu mode.

Press key to allow entry into the displayed menu.

Press key to exit the current setting menu.

Step 2: Press key when appears on the display, the display will show F=0050. This means the system enter the CAL setting menu.

This menu item is used to set the full capacity and main unit of the scale.


Press key to select the main unit lb or kg.

If a different full capacity value is desired, enter the new value via the numeric keypad. Please refer to section 3.3.4 about how to input data of

"FBx Indicator Manual".

FBx-C counting indicator can use numeric keypad, FBx-W weighing

indicator can use





key to shift 1.

Values entered refer to Appendix D for typical values of "FBx Indicator Manual".

Step 3: The full Capacity and main unit are set, press



key to confirm


the setting. The display will show



This menu item is used to set the calibration weight and calibration unit.

If a different calibration weight is desired, enter the new value via the numeric keypad. Please refer to section 3.3.4 about how to input data of "FBx Indicator Manual".

FBx-C counting indicator can use numeric keypad, FBx-W weighing





key to add 1 and



key to shift 1.



key to select the calibration unit lb or kg.

Note: Calibration value range from 1 kilogram or 1 pound to 100% full scale are accepted. Suggest that value range is not less than half of 100% full capacity. Note that values closer to the full capacity will usually yield the most accurate calibration.

Step 4: Calibration weight and unit are set, press



key to confirm the

setting. The display will show



This item is set the division. The unit shown is the main unit that is set in front.

Selections are: 0.01 /0.02 /0.05 /0.1/ 0.2 /0.5 /1 /2 /5 /10 /0.002 /0.005.

After setting the division, the scale will enter the calibration.

Set capacity, main unit, calibration weight, calibration unit and division in sequence. Refer to 3.6 of "FBx Indicator Manual".

Step 5: The division is set, press key to confirm the setting. The display will show a series of digits known as the A/D value.

For example , these numbers will continuously move.

Step 6: Once the display shows the stable indicator "
", press the key, the display will show the calibration weight that you entered in the upper step 3, flashing.

Step 7: Place the corresponding mass on the platform, after 2 seconds,

stable indicator " is displayed, then press the key the scale will calibrate.

If calibration was successful, the calibration weight is displayed and the scale automatically return to the weighing mode. Remove the mass and begin weighing operations.


If calibration fails, please press key to return, then to check if parameter setting is correct.

Step 8:Turn off the power, then turn on the power again, place a known weight on the platform to verify if it is accurate.

Step 9: If the weight displayed does not correspond with the value of the calibration weight, please repeat above steps.

Step 10: After calibration is completed, open the CAL jumper of J13, re-install the front cover and make sure the liquid-tight connector is tight.

Menu flow chart is shown below

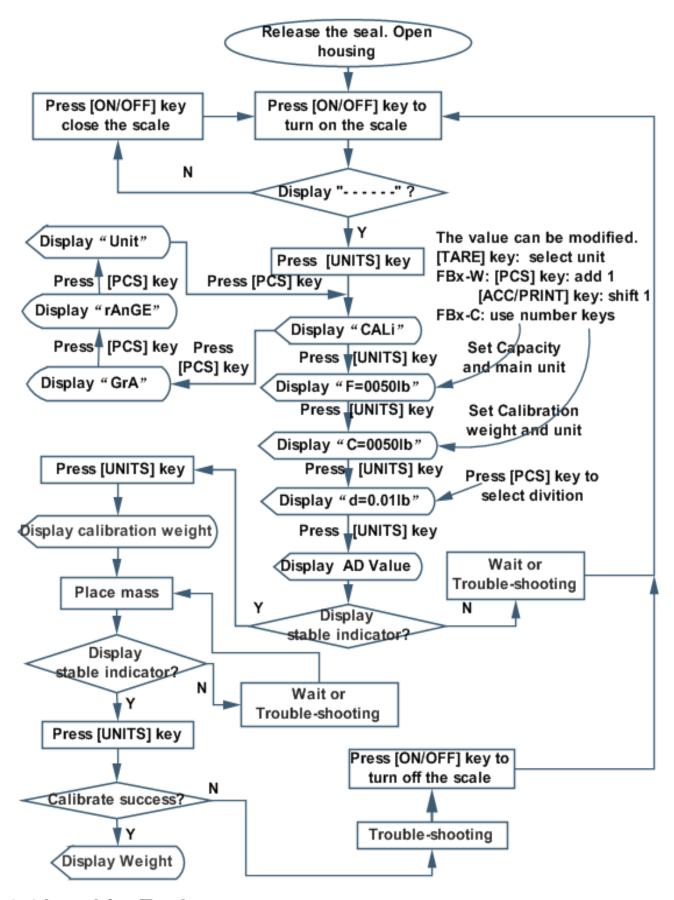

3.4 Legal for Trade

Before this product can be used in legal-for-trade or legally controlled applications, it must be inspected in accordance with local Weights and Measures or approval agency regulations. It is the responsibility of the purchaser to ensure that all pertinent legal requirements are met. Please contact your local Weights and Measures office or authorized manufacturer's representative for further details.

This procedure must only be performed by authorized personnel.

Note: If the scale has been previously set for Legal For Trade operation, it will be necessary to remove the seal before proceeding. Removal of the existing seal will make the scale legally unusable for Legal for Trade use until a new seal is put into place.

4. ACCESSORIES AND OPTIONS

Accessories and Options		
Table/Wall Mounting Bracket		
Table Mounting Kit		
Wall Mounting Kit		
Power Adapter		
USB Cable (option)		
RS232 Cable (option)		

LIMITED WARRANTY

FBx Series Bench Scale

EN-17

Furi products are warranted against defects in materials and workmanship

from the date of delivery through the duration of the warranty period.

During the warranty period Furi will repair, or, at its option, replace any

component(s) that proves to be defective at no charge, provided that the

product is returned, freight prepaid to Furi.

This warranty does not apply if the product has been damaged by accident

or misuse, exposed to radioactive or corrosive materials, has foreign

material penetrating to the inside of the product, or as a result of service or

modification by other than Furi. In lieu of a properly returned warranty

registration card, the warranty period shall begin on the date of shipment

to the authorized dealer. No other express or implied warranty is given by

Furi Corporation. Furi Corporation shall not be liable for any consequential

damages.

As warranty legislation differs from state to state and country to country,

please contact LW Measurements LLC.

USA

LW Measurements LLC,

620 Carlson Court,

Rohnert Park, CA 94928

USA

Tel: +1-707-542-2185

Fax: +1-707-542-3285

Cell: +1-707-480-7406

http://lwmeasurements.com

LW Measurements, LLC

Warranty card

Customer service hotline: 707-542-2185

After-sale service email: support@lwmeasurements.com

Notice: Warranty card helps ensure equipment maintenance service.

Please save the warranty card carefully after opening the carton and using our scale.

User name:				
Address:				
Contacts:	Tel: _		Postcode:	
Purchase Date:		Model Number:		
Device number SNR		Invoice number	 :	

■Users must fill it in correctly for our file to facilitate maintenance

services.

■We will provide maintenance service according to your warranty card and invoice.

Fuzhou Furi Electronics.,LTD

Delivery address: 37 Building, B zone, Pushang Park, Jinshan Industrial

District, Fuzhou

Post code: 350008

Tel: 86-591-83646863,83859705

Fax: 86-591-87984861 ,83050562

Product standard code:

Technology subject to change without notice.

Welcome to visit our company website for more product information.

http://www.furiscale.com



1990101E20801

P/N 1990101E20801 © 2016 Fuzhou Furi Electronics.,LTD property in copyright

No. 00000199 MADE IN FUJIAN